



Allmendstrasse 6 CH-8320 Fehraltorf Tel. +41 43 204 01 01 sales@exista.ch Fax +41 43 204 01 02 www.exista.ch

VER : A_8 update : 2021.04.01

120 Watts

AC-DC Medical Switching Power Supply

MQF1200 SERIES

KEY FEATURES

- Open Frame Medical Switching Power Supply
- Cooling by Free Air Convection
- 100 Watts and 120 Watt with 10CFM Forced Air
- 4000VAC Input to Output 2MOPP Insulation
- High Efficiency up to 91%
- With P.F.C. Function >0.9
- <0.3W No Load Input Power</p>
- EMI for Both Class I (with PE) and Class II (without PE) Configuration
- Suitable for BF Application with Appropriate System Consideration
- UL / IEC / EN 60601 3.1 Edition Safety Approvals
- 3-Year Product Warranty





ELECTRICAL SPECIFICATIONS

All specifications valid at normal input voltage, full load and +25°C after warm-up time unless otherwise stated.

| Model No. | | MQF120O-12S | MQF1200-24S | MQF120O-48S | |
|--------------|---------------------------------------|--|-------------|-------------|--|
| Max Output W | /attage (with 10CFM FAN) (W) | 120 W | | | |
| Max Output W | /attage (Free air Convection) (W) | 100 W | | | |
| Input | Voltage (Note 3) | 90-264 VAC | | | |
| | Frequency (Hz) | 47-63 Hz | | | |
| | Current (Full load) | < 2.0 A max. (115 VAC) / < 1.0 A max. (230 VAC) | | | |
| | Inrush Current (<2ms) | < 40 A max. (115 VAC) / < 70 A max. (230 VAC) | | | |
| | Leakage Current | < 0.1mA / 264 VAC (Touch Current) | | | |
| | Power Factor (at 230 VAC) | PF>0.9 at Full Load | | | |
| | No Load | < 0.3W (115 / 230 VAC) | | | |
| | Voltage (V.DC.) | 12V | 24V | 48V | |
| | Voltage Adj Range (V.DC.) | ±10% Output Voltage | | | |
| | Voltage Accuracy | ±2% | | | |
| | Current (with 10CFM FAN) (A) max | 10 | 5 | 2.5 | |
| | Current (Free air Convection) (A) max | 8.333 | 4.167 | 2.083 | |
| Output | Line Regulation | ±1% | | | |
| Output | Load Regulation (10-100%) | ±1% | | | |
| | Minimum Load | 0% | | | |
| | Maximum Capacitive Load | 3000µF | 1500µF | 500µF | |
| | Ripple & Noise (max.) (Note 1) | 160mV | 1% Vout | | |
| | Efficiency (at 230VAC) | 90% | 90% | 91% | |
| | Hold-up Time (at 115 VAC) (Note 2) | 10 ms min. | | | |
| | Over Power Protection | Auto recovery, Hiccup mode | | | |
| Protection | Over Voltage Protection | Latch off | | | |
| | Over Temperature Protection | Latch off | | | |
| | Short Circuit Protection | Protection level 1 (nominal) : Continuous, Auto recovery | | | |
| | | Protection level 2 (instantaneous high current) : Latch | | | |
| Isolation | Input-Output | 4000VAC or 5656VDC | | | |
| | Input-FG | 2000VAC or 2828VDC | | | |
| | Output-FG | 1500VAC or 2121VDC | | | |





Allmendstrasse 6 CH-8320 Fehraltorf Tel. +41 43 204 01 01 sales@exista.ch Fax +41 43 204 01 02 www.exista.ch

VER : A_8 update : 2021.04.01

AC-DC Medical Switching Power Supply

MQF1200 SERIES

120 Watts

ELECTRICAL SPECIFICATIONS

All specifications valid at normal input voltage, full load and +25°C after warm-up time unless otherwise stated.

| Model No. | | | MQF120O-12S | MQF120O-24S | MQF120O-48S | | |
|-------------|---------------------------|----------|---|-----------------------------|--------------------------|--|--|
| Environment | Operating Temperature | | -30°C+70°C (with derating) | | | | |
| | Storage Temperature | | -30°C+85°C | | | | |
| | Temperature Coefficient | | ±0.05%/°C | | | | |
| | Altitude During Operation | | 5000m | | | | |
| | Humidity | | 20~90% RH | | | | |
| | Atmospheric Pressure | | 56 kPa to 106 kPa | | | | |
| | MTBF | | >250,000 h @ 25°C (MIL-HDBK-217F, Notice 1) | | | | |
| | Vibration | | IEC60068-2-6 (10~500H | z, 2G 10min./1cycle, 60min. | each along X, Y, Z axes) | | |
| | Shock | | IEC60068-2-27 | | | | |
| | Dimensions (L x W x H) | | 3.04 x 2.0 x 1.2 Inches (77.2 x 50.8 x 30.7 mm) Tolerance ±0.5 mm | | | | |
| Physical | Weight | | 172 g | | | | |
| | Cooling Method | | Free convection / 10 CFM FAN | | | | |
| Safety | Approval | | UL / IEC / EN 60601 3.1 rd Edition (2 x MOPP) | | | | |
| EMC | Conducted EMI | (Note 5) | EN55011 Conducted Class B | | | | |
| | Radiated EMI | (Note 5) | EN55011 Class I class B / Class II class A | | | | |
| | EMS | | EN60601-1-2 4th edition | | | | |

NOTE


1. Ripple & Noise are measured at 20MHz of bandwidth with 0.1uF & 47uF parallel capacitor.

- 2. Hold-up Time measured at 90% Vout.
- 3. Please check the derating curve for more details.
- 4. Strongly recommend to conduct this test with AC Voltage. If customer wishes to test with DC Voltage, please disconnect all Y-Capacitors from Arch power supply.
- 5. Please secure the power supply unit to your metal case by using the four screw holes in the corners for either Class I or Class II equipment
- 6. CAUTION: Double pole, neutral fusing. Disconnect mains before servicing.

(ATTENTION : 2 poles avec fusible sur le neutre. Deconnecter le secteur avant intervention.)

DERATING

If the input voltage is below 99VAC, the product can be used only in an environment where temperature is higher than -10 degrees Celsius.

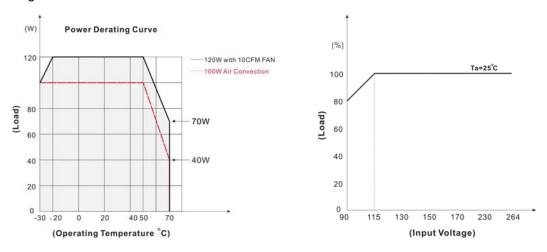






Allmendstrasse 6 CH-8320 Fehraltorf Tel. +41 43 204 01 01 sales@exista.ch Fax +41 43 204 01 02 www.exista.ch

VER : A_8 update : 2021.04.01

AC-DC Medical Switching Power Supply


MQF1200 SERIES

MECHANICAL DIMENSIONS (Top View)

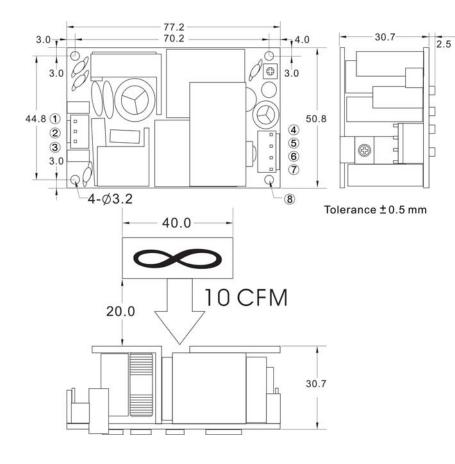

| Brands | | AI | ex | JST | | |
|--------|-----------|-------------------|------------|-------------------|--------------|--|
| PIN# | Single | Mating Housing | Terminal | Mating Housing | Terminal | |
| 1 | AC IN (N) | 9396-3 | 96T series | VHR-3N | SVH-41T-P1.1 | |
| 2 | NO PIN | | | | | |
| 3 | AC IN (L) | | | | | |
| 4~5 | +DC OUT | 0000 4 | 96T series | VHR-4N | SVH-41T-P1.1 | |
| 6~7 | -DC OUT | 9396-4 | | | | |
| 8 | PE | | | | | |

BLOCK DIAGRAM

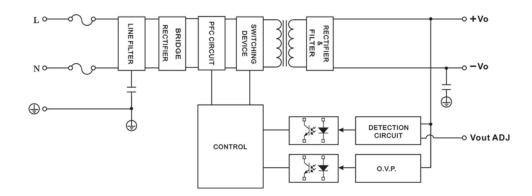

-3-